

Before you begin

- Please read the instructions for use in its entirety, prior to use.
- Cover your work space with a clean, disposable absorbent workspace cover.
- All components and specimen must be brought to room temperature (between 15-30°C) prior to testing.
- Do not use the test more than once.

Preparation


- Test pouch (test device)
- Assay diluent (for Dengue IgG/IgM)
- Disposable capillary pipette (10 µl) (for Dengue IgG/IgM)
- Disposable dropper (for Dengue NS1 Ag)
- Timer & disposable gloves (not provided)

For more detailed instructions please refer to Instructions for use.



1 Check the expiration date.
If the device is expired, use another kit.



2 Put on disposable gloves.
Use new gloves for each patient.




3 Open the test pouch and write the patient's name on the test device.

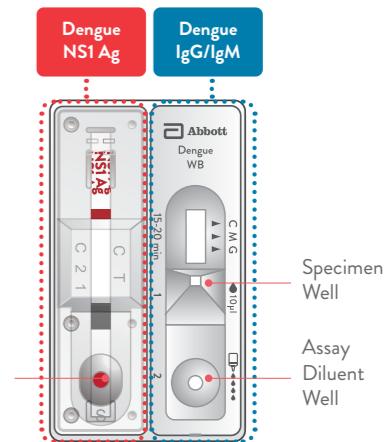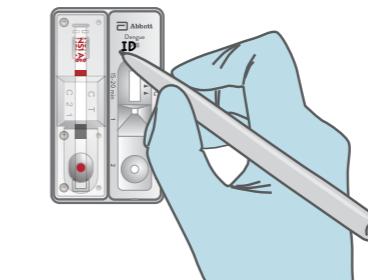


4 **DENGUE NS1 Ag**
Add 3 drops (100 µl) of specimen into the specimen well ("S").
Discard the dropper in the biohazard box after use.



5 **DENGUE IgG/IgM**
Draw specimen to **black line** (10 µl) then add into the square specimen well (►10 µl).
Discard the pipette in the biohazard box after use.

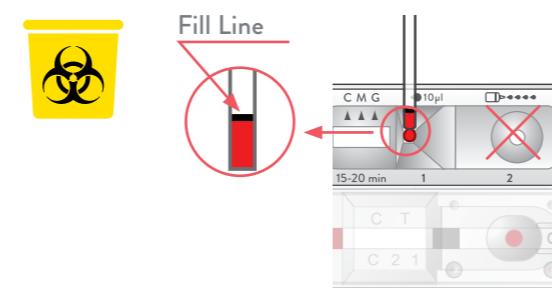

6 **DENGUE IgG/IgM**
Add 4 drops of assay diluent into the round assay diluent well (►•••••).

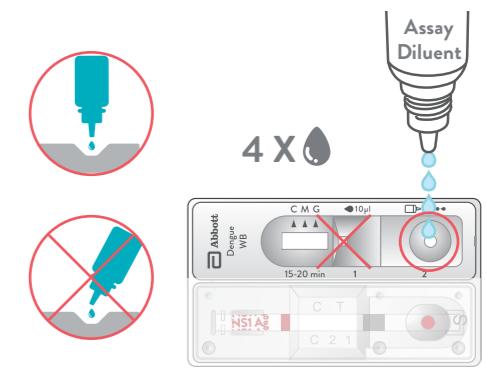

7 Read results between 15-20 minutes after adding diluent.




Do not read after 20 minutes.
Reading outside of this time frame may provide false results.

Caution: Visible test lines should be considered positive, even if faint.

NEGATIVE




POSITIVE

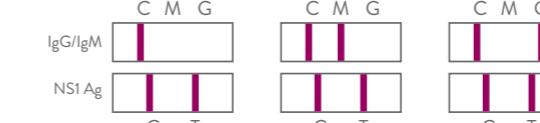

INVALID



The control line should appear for all results. If it does not appear, the result is considered invalid and the specimen should be retested using a new test kit.

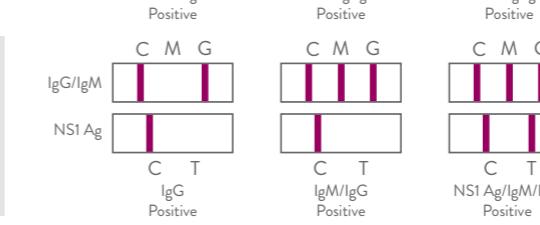

FOR TECHNICAL SUPPORT PLEASE VISIT ABBOTT.COM/POCT